

VIASURE

Real Time PCR Detection Kit



***SARS-CoV-2 Variant II
(P681R+L452R) Real Time PCR
Detection Kit for BD MAX™ System***

CE IVD



These instructions for use apply to the following reference / Denne brugsanvisning gælder for følgende reference:

PRODUCT / PRODUKT	REFERENCE / REFERENCE
VIASURE SARS-CoV-2 Variant II (P681R+L452R) Real Time PCR Detection Kit for BD MAX™ System	444218 / VS-VAD124

Table A 1. Reference for product to be used with the BD MAX™ System. / Reference til produkt, der skal bruges med BD MAX™ System.

Content

1.	Intended use.....	5
2.	Summary and Explanation	5
3.	Principle of the procedure	6
4.	Reagents provided	6
5.	Reagents and equipment to be supplied by the user	7
6.	Transport and storage conditions.....	7
7.	Precautions for users	7
8.	Test procedure	8
8.1.	Sample collection, storage and transport.....	8
8.2.	Sample preparation and RNA extraction.....	9
8.3.	PCR protocol	9
9.	Result interpretation	13
10.	Limitations of the test	15
11.	Quality control	16
12.	Performance characteristics.....	16
12.1.	Clinical sensitivity and specificity	16
12.2.	Analytical sensitivity	18
12.3.	Analytical specificity	18
12.4.	Analytical reactivity	19

Indholdsfortegnelse

1.	Anvendelsesformål	20
2.	Oversigt og forklaring.....	20
3.	Procedurens princip.....	21
4.	Leverede reagenser	21
5.	Reagenser og udstyr, der skal leveres af brugeren	22
6.	Transport- og opbevaringsforhold.....	22
7.	Særlige forholdsregler for brugere	22
8.	Analysemetode.....	23
8.1.	Prøveindsamling, opbevaring og transport.....	23
8.2.	Prøveklargøring og RNA-ekstraktion.....	24
8.3.	PCR-protokol.....	24

9.	Tolkning af resultater	28
10.	Begrænsninger i testen.....	30
11.	Kvalitetskontrol.....	31
12.	Ydelseskarakteristika	32
12.1.	Klinisk sensitivitet og specificitet	32
12.2.	Analytisk sensitivitet	33
12.3.	Analytisk specificitet.....	34
12.4.	Analytisk reaktivitet	35
	Bibliography/ Bibliografi.....	36
	Symbols for IVD components and reagents/ Symboler for IVD-komponenter og -reagenser.....	37
	Trademarks.....	37

ENGLISH

1. Intended use

VIASURE SARS-CoV-2 Variant II (P681R+L452R) Real Time PCR Detection Kit for BD MAX™ System is an automated real-time RT-PCR test designed for the qualitative detection of P681R mutation and L452R mutation in the S gene RNA from positive SARS-CoV-2 nasopharyngeal and oropharyngeal swabs and saliva samples.

The assay is intended to be used with SARS-CoV-2 positive samples or, when the test is performed in conjunction with the VIASURE SARS-CoV-2 (N1 + N2) Real Time PCR Detection Kit for BD MAX™ System (Ref: 444215) with samples from patients suspected Coronavirus disease 2019 (COVID-19) by their healthcare professional (HCP).

This test is intended to be used as an aid to monitor the prevalence of P681R or L452R mutations in the S gene and to assist in control measures. The assay uses the BD MAX™ System for automated extraction of RNA and subsequent real-time RT-PCR, employing the reagents provided combined with universal reagents and disposables for the BD MAX™ System. RNA is extracted from specimens, and complementary DNA (cDNA) is synthesized and amplified using RT-PCR and detected using fluorescent reporter dye probes specific for P681R and L452R mutations.

2. Summary and Explanation

All viruses, including SARS-CoV-2, mutates over time. some changes may affect the virus' properties, such as how easily it spreads, the associated disease severity, or the performance of vaccines, therapeutic medicines, diagnostic tools, or other public health and social measures.

The appearance of genetic mutations is a natural and expected event within the evolution process of a virus. In fact, some specific mutations define the viral genetic groups currently circulating globally. Besides, thanks to the genetic sequencing of the pathogen worldwide, it has been possible to establish patterns of dispersal and evolution of the virus.

At the end of 2020, the appearance of variants with a higher risk for public health prompted the characterization of Variants of Interest (VOI) and Variants of Concern (VOC), in order to facilitate epidemiological control. Some of these SARS-CoV-2 variants are:

Delta (B.1.617.2 lineage) and Kappa (B.1.617.1 lineage) variants were closely associated with a huge COVID-19 increase in India during Spring 2021. Delta variant has multiple mutations in the Spike protein, including P681R and L452R. Kappa variant has also genetic mutations in the Spike protein, including P681R, L452R and E484Q.

All these mutations described above show potential reduction in neutralization by some immunotherapies and reduction of expected effects of vaccines or has been identified to cause community transmission.

That is why, the appearance of variants that increase the transmissibility of the virus, its virulence or that escape the action of the neutralizing antibodies generated after natural infection or the vaccine, constitute a first-order public health problem that can have an important impact on control of the pandemic.

For this reason, VIASURE SARS-CoV-2 Variant II (P681R+L452R) Real Time PCR Detection Kit for BD MAX™ System has been designed to allow the detection of the main mutation associated with the variant under surveillance.

3. Principle of the procedure

VIASURE SARS-CoV-2 Variant II (P681R+L452R) Real Time PCR Detection Kit for BD MAX™ System is designed for the qualitative detection of RNA with P681R and L452R mutations in the *S* gene of SARS-CoV-2 from positive nasopharyngeal and oropharyngeal swabs and saliva samples. The detection is done in one step real-time RT-PCR format where the reverse transcription and the subsequent amplification of specific target sequence occur in the same reaction tube. The isolated RNA target is transcribed generating complementary DNA by reverse transcriptase, which is followed by the amplification of a conserved region of *S* gene of SARS-CoV-2 for P681R mutation and L452R mutation using specific primers and fluorescent-labelled probes.

VIASURE SARS-CoV-2 Variant II (P681R+L452R) Real Time PCR Detection Kit for BD MAX™ System is based on 5' exonuclease activity of DNA polymerase. During DNA amplification, this enzyme cleaves the probe bound to the complementary DNA sequence, separating the quencher dye from the reporter. This reaction generates an increase in the fluorescent signal which is proportional to the quantity of the target template. This fluorescence is measured on the BD MAX™ System.

VIASURE SARS-CoV-2 Variant II (P681R+L452R) Real Time PCR Detection Kit for BD MAX™ System contains in each tube all the components necessary for real-time PCR assay (specific primers/probes, dNTPs, buffer, polymerase, reverse-transcriptase) in a stabilized format, as well as an endogenous internal control to monitor the extraction process and/or inhibition of the polymerase activity. The assay uses a human housekeeping gene as an Endogenous Internal Control (IC) (human *RNase P* gene). Human housekeeping genes are involved in basic cell maintenance and, therefore, are expected to be present in all nucleated human cells and maintain relatively constant expression levels.

Target	Channel	Gene
P681R mutation	475/520	<i>S</i> gene
L452R mutation	530/565	<i>S</i> gene
Endogenous Internal Control (IC)	585/630	human <i>RNase P</i> gene

Table 1. Target, channel and genes.

4. Reagents provided

VIASURE SARS-CoV-2 Variant II (P681R+L452R) Real Time PCR Detection Kit for BD MAX™ System includes the following materials and reagents detailed in Table 2:

Reagent/Material	Description	Color or Barcode	Amount
SARS-CoV-2 Variant II (P681R+L452R) reaction tube	A mix of enzymes, primers-probes, buffer, dNTPs, stabilizers and endogenous internal control in stabilized format	Blue foil	2 pouches of 12 transparent tubes
Rehydration Buffer tube	Solution to reconstitute the stabilized product	11 foil	1 pouch of 24 transparent tubes

Table 2. Reagents and materials provided in VIASURE SARS-CoV-2 Variant II (P681R+L452R) Real Time PCR Detection Kit for BD MAX™ System with Cat. N°. VS-VAD124 (444218).

5. Reagents and equipment to be supplied by the user

The following list includes the materials and equipment that are required for use but not included in the VIASURE SARS-CoV-2 Variant II (P681R+L452R) Real Time PCR Detection Kit for BD MAX™ System.

- Real-time PCR instrument: BD MAX™ System (Ref: 441916).
- BD MAX™ ExK™ TNA-3 (Ref:442827 or 442828).
- BD MAX™ PCR Cartridges (Ref: 437519).
- Vortex.
- Micropipettes (accurate between 2 and 1000 µL).
- Filter tips.
- Powder-free disposable gloves.
- Optional: VIASURE SARS-CoV-2 (N1 + N2) Real Time PCR Detection Kit for BD MAX™ System (Ref: 444215)

6. Transport and storage conditions

- The kits can be shipped and stored at 2-40°C until the expiration date which is stated on the label.
- After opening the aluminium pouches which contain the reaction tubes, the product can be used up to 28 days.

7. Precautions for users

- The product is intended for use by professional users only, such as laboratory or health care professionals and technicians, trained in molecular biological techniques.
- For *in vitro* diagnostic use.
- Do not use expired reagents and/or materials.
- Do not use the kit if the label that seals the outer box is broken.
- Do not use reagents if the protective box is open or broken upon arrival.
- Do not use reagents if the protective pouches are open or broken upon arrival.
- Do not use reagents if desiccant is not present or broken inside reagent pouches.
- Do not remove desiccant from reagent pouches.
- Close protective pouches of reagents promptly with the zip seal after each use. Remove any excess air in the pouches prior to sealing.
- Do not use reagents if the foil has been broken or damaged.
- Do not mix reagents from different pouches and/or kits and/or lots.
- Protect reagents from humidity. Prolonged exposure to humidity may affect product performance.
- Keep components away from light.
- In cases where other PCR tests are conducted in the same general area of the laboratory, care must be taken to ensure that the VIASURE SARS-CoV-2 Variant II (P681R+L452R) Real Time PCR Detection Kit for BD MAX™ System, BD MAX™ ExK™ TNA-3 extraction kit, any additional reagents required for testing and the BD MAX™ System are not contaminated. Always avoid microbial and ribonuclease (RNase)/deoxyribonuclease (DNase) contamination of reagents. The use of sterile RNase/DNase-free disposable aerosol resistant or positive

displacement pipette tips is recommended. Use a new tip for each specimen. Gloves must be changed before manipulating reagents and cartridges (BD MAX™ PCR Cartridge).

- To avoid contamination of the environment by amplicons, do not break apart the BD MAX™ PCR Cartridge after use. The seals of the BD MAX™ PCR Cartridge are designed to prevent contamination.
- Design a unidirectional workflow. It should begin in the Extraction Area and then move to the Amplification and Detection Area. Do not return samples, equipment and reagents to the area in which the previous step was performed.
- Follow Good Laboratory Practices. Wear protective clothing, use disposable gloves, goggles and mask. Do not eat, drink, smoke or apply cosmetic products in the working area. Wash your hands after finishing the test.
- Samples must be treated as potentially infectious and/or biohazardous, as well as all the reagents and materials that have been exposed to the samples and they must be handled according to the national safety regulations. Take necessary precautions during the collection, transport, storage, handling, and disposal of samples.
- Samples and reagents must be handled in a biological safety cabinet. Use personal protective equipment (PPE) consistent with current guidelines for the handling of potentially infectious samples. Dispose of waste in compliance with local and state regulations.
- Regular decontamination of commonly used equipment is recommended, especially micropipettes and work surfaces.
- In accordance with Regulation (EC) No 1907/2006 (REACH), VIASURE Real Time PCR Detection Kits do not require Material Safety Data Sheets on account of their classification as non-hazardous to health and the environment, because they do not contain substances and/or mixtures which meet the hazard classification criteria available in Regulation (EC) No 1272/2008 (CLP), or which are in concentrations higher than the value established in the mentioned regulation for their declaration.
- If the kit is used in combination with the VIASURE SARS-CoV-2 (N1 + N2) Real Time PCR Detection Kit for BD MAX™ System (Ref: 444215), please refer to the corresponding instructions for use.
- Consult the BD MAX™ System User's Manual for additional warnings, precautions and procedures.

8. Test procedure

8.1. Sample collection, storage and transport

The VIASURE SARS-CoV-2 Variant II (P681R+L452R) Real Time PCR Detection Kit for BD MAX™ System has been tested on nasopharyngeal swabs and saliva samples, both collected in viral transport medium (VTM) – Vircell S.L. -; BD™ Universal Viral Transport (UVT) System media – BD - or IMPROVIRAL™ Viral Preservative Medium (VPM) -Guangzhou Improve Medical Instruments Co. Ltd and oropharyngeal swabs collected in viral transport medium (VTM) - Vircell. Other types of samples must be validated by the user.

Collection, storage and transport of specimens should be maintained per the conditions validated by the user. Overall, respiratory and saliva samples should be collected and labelled appropriately in clean containers with or without transport media (depending on sample type) and processed as soon as possible to guarantee the quality of the test. The specimens should be transported at 2 to 8°C for up to 72 hours, following the local and national regulations for the transport of pathogen material. For long term transport (more than 72 hours), we recommend

shipping at $\leq -20^{\circ}\text{C}$ or lower. It is recommended to use fresh specimens for the test. The samples can be stored at 2 to 8°C for up to 72 hours or frozen at -20°C or ideally at -70°C for conservation. Repeated freeze-thaw cycles should be avoided in order to prevent degradation of the sample and nucleic acids.

The nasopharyngeal/oropharyngeal swabs and saliva specimens must be collected, transported and stored according to appropriate laboratory guidelines. For details, refer to the CDC guideline (Specimen collection guidelines. Website <https://www.cdc.gov/urdo/downloads/SpecCollectionGuidelines.pdf> and Interim Guidelines for Collecting, Handling, and Testing Clinical Specimens for COVID-19. Website <https://www.cdc.gov/coronavirus/2019-ncov/lab/guidelines-clinical-specimens.html>) and the IDSA guideline (Miller, J. M., Binnicker, M. J., Campbell, S., ... & Pritt, B. S. (2018). A guide to utilization of the microbiology laboratory for diagnosis of infectious diseases: 2018 update by the Infectious Diseases Society of America and the American Society for Microbiology. *Clinical Infectious Diseases*, 67(6), e1-e94).

8.2. Sample preparation and RNA extraction

Perform the sample preparation according to the recommendations in the instructions for use of extraction kit used, BD MAX™ ExK™ TNA-3. Note that some other samples may require pre-processing. Application-specific extraction preparation procedures should be developed and validated by the user.

When using nasopharyngeal or oropharyngeal specimens:

1. Pipette between 400 and 750 μL of nasopharyngeal or oropharyngeal swab collected in viral transport media (VTM), BD™ Universal Viral Transport (UVT) System media or IMPROVIRAL™ Viral Preservative Medium (VPM) into a BD MAX™ ExK™ TNA-3 Sample Buffer Tube and close the tube with a septum cap. Ensure complete mixing by vortexing the sample at high speed for 1 minute. Proceed to BD MAX™ System Operation.

In case of using saliva samples collected in transport media:

1. Saliva samples may be collected in Viral Transport Medium (VTM), BD™ Universal Viral Transport (UVT), or IMPROVIRAL™ Viral Preservative Medium (VPM) at a ratio of 1:3 (saliva:media). Vortex for 1 minute at high speed. Pipette 750 μL into a BD MAX™ ExK™ TNA-3 Sample Buffer Tube and close the tube with a septum cap. Ensure complete mixing by vortexing the sample at high speed for 1 minute. Proceed to BD MAX™ System Operation.

In case of using neat saliva samples:

1. Combine saliva with Viral Transport Medium (VTM), BD™ Universal Viral Transport (UVT), or IMPROVIRAL™ Viral Preservative Medium (VPM) so that the final ratio of saliva:media is 1:3. Vortex for 1 minute at high speed. Then pipette 750 μL into a BD MAX™ ExK™ TNA-3 Sample Buffer Tube and close the tube with a septum cap. Ensure complete mixing by vortexing the sample at high speed for 1 minute. Proceed to BD MAX™ System Operation.

8.3. PCR protocol

Note: Please, refer to the BD MAX™ System User's Manual for detailed instructions.

8.3.1. Creating PCR test program for VIASURE SARS-CoV-2 Variant II (P681R+L452R) Real Time PCR Detection Kit for BD MAX™ System

Note: If you have already created the test for the VIASURE SARS-CoV-2 Variant II (P681R+L452R) Real Time PCR Detection Kit for BD MAX™ System, you can skip step 8.3.1 and go directly to 8.3.2.

- 1) On the "Run" screen of the BD MAX™ System, select the "Test Editor" tab.
- 2) Click the "Create" button.
- 3) In the Basic Information tab, within the "Test Name" window, name your test: i.e. VIASURE SARS-CoV-2 Variant II (P681R+L452R).
- 4) In the "Extraction Type" drop down menu, select "ExK TNA-3".
- 5) In the "Master Mix Format" drop down menu, choose "Type 5".
 - a. Note: Product may be used in combination with the VIASURE SARS-CoV-2 (N1 + N2) Real Time PCR Detection Kit for BD MAX™ System (Ref: 444215), then select "Dual Master Mix Concentrated Lyophilized MM with Rehydration Buffer (Type 5)".
- 6) In the "Sample extraction parameters" select "User defined" and adjust sample volume to 950 µL.
- 7) In the "Ct Calculation" select "Call Ct at Threshold Crossing".
- 8) If running software version 5.00 or higher, in the "Custom Barcodes" select the following configuration:
 - a. Snap-In 2 Barcode: leave empty (concerning SARS-CoV-2 Variant II (P681R+L452R) reaction tube no barcode configuration is needed).
 - b. Snap-In 3 Barcode: 11 (concerning Rehydration Buffer tube).
 - c. Snap-In 4 Barcode: 1G if used in combination with SARS-CoV-2 (N1 + N2) reaction tube and the format "Dual Master mix Concentrated Lyophilized MM with rehydration Buffer (Type 5)" (Section 8.3.1).
- 9) In "PCR settings" tab enter the following parameters: "Channel Settings", "Gains" and "Threshold" (Table 3).
 - a. Note: Product may be used in combination with the VIASURE SARS-CoV-2 (N1 + N2) Real Time PCR Detection Kit for BD MAX™ System (Ref: 444215), "PCR Settings" and "Test Steps" should be completed for Snap-In 4 (blue) position (see the corresponding instructions for use).

Channel	Alias	Gain	Threshold	Ct Min	Ct Max
475/520 (FAM)	P681R	80	150	0	40
530/565 (HEX)	L452R	80	150	0	40
585/630 (ROX)	IC	80	150	0	35
630/665 (Cy5)	-	0	0	0	0
680/715 (Cy5.5)	-	0	0	0	0

Table 3. PCR settings.

Note: It is recommended to set the minimum threshold values listed above for each channel as a starting point, but the final settings must be determined by the end-user during the result interpretation, in order to ensure that thresholds fall within the exponential phase of the fluorescence curves and above any background signal. The threshold value for different instruments may vary due to different signal intensities.

- 10) In "PCR settings" tab enter the following parameters "Spectral Cross Talk" (Table 4), as well.

		False Receiving Channel				
Channel		475/520	530/565	585/630	630/665	680/715
Excitation Channel	475/520	-	3.0	0.0	0.0	0.0
	530/565	1.0	-	0.0	0.0	0.0
	585/630	0.0	0.0	-	0.0	0.0
	630/665	0.0	0.0	0.0	-	0.0
	680/715	0.0	0.0	0.0	0.0	-

Table 4. Spectral cross-talk parameters.

- 11) In "Test Steps" tab, enter the PCR protocol (Table 5).

Step Name	Profile Type	Cycles	Time (s)	Temperature	Detect
Reverse transcription	Hold	1	900	45°C	-
Initial denaturation	Hold	1	120	98°C	-
Denaturation and Annealing/Extension (Data collection)	2-Temperature	45	10	95°C	-
			61.1	63°C	✓

Table 5. PCR protocol.


- 12) Click the "Save Test" button.

8.3.2. BD MAX™ Rack set up

- For each sample to be tested, remove one Unitized Reagent Strips from the BD MAX™ ExK™ TNA-3 kit. Gently tap each strip onto a hard surface to ensure that all the liquids are at the bottom of the tubes and load on the BD MAX™ System sample racks.
- Remove the required number of BD MAX™ ExK™ TNA Extraction Tubes (B4) (white foil) from their protective pouch. Snap the Extraction Tube(s) (white foil) into its corresponding positions in the TNA strip (Snap position 1, white color coding on the rack. See Figure 1). Remove excess air, and close pouch with the zip seal.
- Determine and separate the appropriate number of SARS-CoV-2 Variant II (P681R+L452R) reaction tubes (blue foil) and snap into their corresponding positions in the strip (Snap position 2, green color coding on the rack. See Figure 1).
 - Remove excess air, and close aluminium pouches with the zip seal.
 - In order to carry out a correct rehydration, please make sure that the lyophilized product is in the bottom of the tube and is not adhered to the top area of the tube or to the foil seal. Gently tap each tube on a hard surface to make sure all the product is at the bottom of the tube.
 - Note: If you choose the format "Dual Master Mix Concentrated Lyophilized MM with Rehydration Buffer (Type 5)" (Section 8.3.1), determine and separate the appropriate number of additional SARS-CoV-2 reaction tubes (1G foil in case of VIASURE SARS-CoV-2 (N1+N2) test) and snap into their corresponding positions in the strip (Snap position 4, blue color coding on the rack. See Figure 1). Remove excess air, and close aluminium pouches with the zip seal.

- 4) Remove the required number of Rehydration Buffer tubes (11 foil) and snap into their corresponding positions in the strip (Snap position 3, non-color coding on the rack. See Figure 1). Remove excess air and close the pouch with the zip seal.
 - a. In order to ensure a correct transfer, please make sure that the liquid is in the bottom of the tube and is not adhered to the top area of the tube or to the foil seal. Gently tap each tube on a hard surface to make sure all the buffer is at the bottom of the tube.

Figure 1. BD MAX™ TNA Reagent Strip (TNA) from the BD MAX™ ExK™ TNA-3 kit.

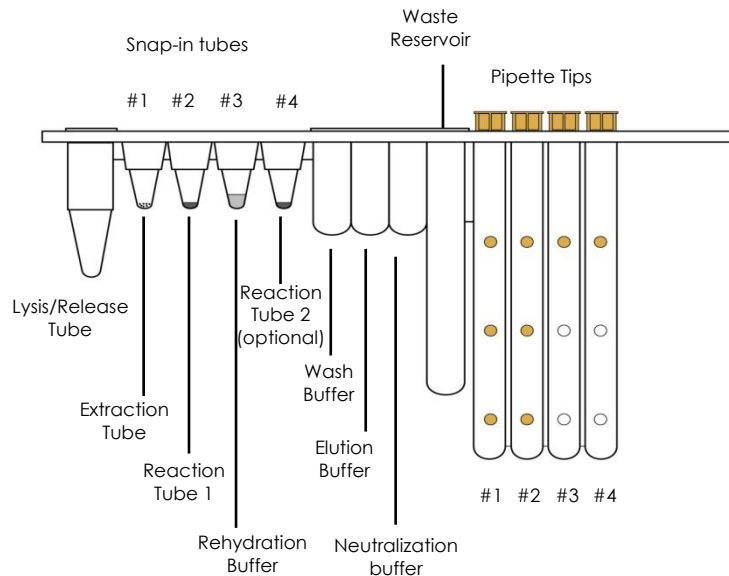

8.3.3. BD MAX™ Instrument set up

- 1) Select the "Work List" tab on the "Run" screen of the BD MAX™ System software v4.50A or higher.
- 2) In the "Test" drop down menu, select *VIASURE SARS-CoV-2 Variant II (P681R+L452R)* (if not already created see Section 8.3.1).
- 3) Select the appropriate kit lot number (found on the outer box of extraction kit used) from the pull-down menu (optional).
- 4) Enter the Sample Buffer Tube identification number into the Sample tube window of the Work List, either by scanning the barcode with the scanner or by manual entry.
- 5) Fill the Specimen/Patient ID and/or Accession window of the Work List and click the "Save" button. Continue until all Sample Buffer Tubes are entered. Ensure that the specimen/patient ID and the Sample Buffer Tubes are accurately matched.
- 6) Place the prepared Sample Buffer Tube into the BD MAX™ Rack(s).
- 7) Load the rack(s) into the BD MAX™ System (Rack A is positioned on the left side of the BD MAX™ System and Rack B on the right side).
- 8) Place the required number of BD MAX™ PCR Cartridge(s) into the BD MAX™ System.
- 9) Close the BD MAX™ System door.
- 10) Click "Start Run" to begin the procedure.

8.3.4. BD MAX™ report

- 1) In main menu, click the "Results" button.
- 2) Either double click on your run in the list or press the "view button".
- 3) Click on "Print", select: "Run Details, Test Details and Plot...".
- 4) Click on "Print or Export button" on the "Run Reports" screen.

9. Result interpretation

For a detailed description on how to analyse data, refer to the BD MAX™ System User's manual.

Analysis of the VIASURE SARS-CoV-2 *Variant II (P681R+L452R)* Real Time PCR Detection Kit for BD MAX™ System is intended to be performed as a reflex on samples with positive result for SARS-CoV-2 RNA. If used in conjunction with VIASURE SARS-CoV-2 (*N1 + N2*) Real Time PCR Detection Kit for BD MAX™ System on samples of unknown status for presence of SARS-CoV-2 RNA, please refer to those instructions for use for results interpretation for determination of the SARS-CoV-2 RNA result.

The analysis of the data is done by the BD MAX™ software according to the manufacturer's instructions. The BD MAX™ software reports Ct values and amplification curves for each detector channel of each sample tested in the following way:

- Ct value of 0 indicates that there was no Ct value calculated by the software with the specified Threshold (see Table 3). Amplification curve of the sample showing a "0" Ct value must be checked manually.
- Ct value of -1 indicates that no amplification process has occurred.
- Any other Ct value should be interpreted in correlation with the amplification curve and according to the sample interpretation guidelines outlined in Table 6.

Check Internal Control signal to verify the correct functioning of the amplification mix. In addition, check that there is no report of BD MAX™ System failure.

Results should be read and analysed using the following table:

P681R mutation target (475/520)	L452R mutation target (530/565)	Endogenous Internal Control (585/630)	Interpretation
+	-	+/- ¹	P681R mutation Detected ¹
-	+	+/- ¹	L452R mutation Detected ¹
+	+	+/- ¹	P681R mutation and L452R mutation Detected ¹
-	-	+ ¹	P681R mutation and L452R mutation Not Detected ¹
-	-	- ²	Unresolved (UNR) Result obtained in the presence of inhibitors in the PCR reaction or when a general problem (not reported by an error code) with the sample processing and/or amplification steps occurs.²
IND	IND	IND	Indeterminate assay result (IND). Due to BD MAX™ System failure. Assay result displayed in case of an instrument failure linked to an error code.
INC	INC	INC	Incomplete assay result (INC). Due to BD MAX™ System failure. Assay result displayed in case of failure to complete run.

Table 6. Sample interpretation.

+: Amplification occurred.

-: No amplification occurred.

1 A sample is considered positive if the Ct value obtained is less than 40. The endogenous Internal Control (IC) may or may not show an amplification signal. Sometimes, the IC detection is not necessary because a high copy number of the target can cause preferential amplification of target-specific nucleic acids.

2 In the case of P681R mutation and L452R mutation targets sites negative, IC must show an amplification signal with Ct less than 35. The Ct value could be very variable due to the Endogenous Internal Control is a human housekeeping gene that should be present in all human nucleated cells in the original sample. If there is an absence of signal or Ct value ≥ 35 of the Endogenous Internal Control, the result is considered as 'Unresolved', and retesting is required.

Summary of mutations associated with the following lineages present in the most known Variants of Concern (VOC):

Lineages	WHO label	Mutations in the S gene ¹	
		P681R	L452R
B.1.617.1	Kappa	X	X
B.1.617.2	Delta	X	X

Table 7. Summary of mutations associated with known Variants of Concern (VOC).

¹Tracking SARS-CoV-2 variants: <https://www.who.int/en/activities/tracking-SARS-CoV-2-variants/> (data up to 02nd September 2021).

²Overview of Variants/Mutations <https://covariants.org/variants> (data up to 02nd September 2021).

Other variants can present the mutations P681R and L452R because they are not specific for the variants mentioned.

Final assignment to a lineage must be done by sequencing.

In case of a continued ambiguous result, it is recommended to review the instructions for use, the extraction process used by the user; to verify the correct performance of each RT-qPCR steps and review the parameters; and to check the sigmoid shape of the curve and the intensity of fluorescence.

The results of the test should be evaluated by a health care professional in the context of medical history, clinical symptoms and other diagnostic tests.

10. Limitations of the test

- The results of the test should be evaluated by a health care professional in the context of medical history, clinical symptoms and other diagnostic tests.
- Although this assay can be used with other types of samples it has been validated with nasopharyngeal/oropharyngeal swabs and saliva samples.
- For good test performance, the lyophilized product should be at the bottom of the tube and not adhered to the top area of the tube or the foil seal. Gently tap each tube on a hard surface to make sure all the product is at the bottom of the tube.
- An appearance of the reaction mixture in stabilized format, normally found at the bottom of the tube, different from the usual one (without conical shape, inhomogeneous, smaller/larger in size and/or color different from whitish) does not alter the functionality of the test.
- The quality of the test depends on the quality of the sample; proper extracted nucleic acid from respiratory samples must be extracted.
- This test is a qualitative test and does not provide quantitative values or indicate the number of organisms present.
- Extremely low levels of target below the limit of detection might be detected, but results may not be reproducible.
- Samples with a Ct value between 35 and 40 might show greater variability in the results obtained.
- There is a possibility of false positive results due to cross-contamination by SARS-CoV-2 RNA with P681R mutation or L452R mutation in the S gene, either samples containing high concentrations of target RNA or contamination due to PCR products from previous reactions.
- The specific primer and probe combinations for detection of P681R mutation or L452R mutation used in VIASURE SARS-CoV-2 Variant II (P681R+L452R) Real Time PCR Detection Kit for BD MAX™ System do not show significant combined homologies with the human genome, human microflora, or other coronaviruses, which might result in predictable false positive.
- False Negative results may arise from several factors and their combinations, including:
 - Improper specimens' collection, transport, storage, and/or handling methods.
 - Improper processing procedures (including RNA extraction).
 - Degradation of the viral RNA during sample shipping/storage and/or processing.
 - Mutations or polymorphisms in primer or probe binding regions may affect detection of new or unknown SARS-CoV-2 variant.
 - A viral load in the specimen below the limit of detection for the assay.
 - The presence of RT-qPCR inhibitors or other types of interfering substances. The impacts of vaccines, antiviral therapeutics, antibiotics, chemotherapeutics or immunosuppressant drugs used to prevent COVID-19 or used during the treatment of the infection have not been evaluated.

- Failure to follow instructions for use and the assay procedure.
- Some samples may fail to exhibit *RNase P* amplification curves due to low human cell numbers in the original clinical sample. A negative IC signal does not preclude the presence of P681R mutation or L452R mutation in a clinical specimen.
- A positive test result does not necessarily indicate the presence of viable viruses and does not imply that these viruses are infectious or are the causative agents for clinical symptoms. However, a positive result is indicative of the presence of targets viral sequences.
- The presence of the P681R and L452R mutations is associated with Kappa (lineage B.1.617.1) and Delta (lineage B.1.617.2) variants, however, final assignment to a lineage must be done by sequencing.
- Negative results do not preclude presence of SARS-CoV-2 RNA due to this assay is intended to be used with positive SARS-CoV-2 samples.
- In the case of obtaining Unresolved, Indeterminate or Incomplete results using VIASURE SARS-CoV-2 Variant II (P681R+L452R) Real Time PCR Detection Kit for BD MAX™ System, retesting will be required. Unresolved results may be due to the presence of inhibitors in the sample or an incorrect rehydration of lyophilized reaction mix tube. If there is an instrument failure, Indeterminate or Incomplete results will be obtained.

11. Quality control

VIASURE SARS-CoV-2 Variant II (P681R+L452R) Real Time PCR Detection Kit for BD MAX™ System contains an Endogenous Internal Control (IC) in each reaction tube which confirms the correct performance of the technique.

12. Performance characteristics

12.1. Clinical sensitivity and specificity

The clinical performance of VIASURE SARS-CoV-2 Variant II (P681R+L452R) Real Time PCR Detection Kit for BD MAX™ System was tested using clinical samples (nasopharyngeal swabs) already characterized as positive or negative for SARS-CoV-2, from patients. The results were as follows:

	Site	Sample type	Workflow	Target
1	CerTest Biotec S.L (Zaragoza, Spain)	nasopharyngeal swab	BD MAX™ EXK™ TNA-3 kit + BD MAX™ System	P681R mutation L452R mutation

Table 8. Site, sample type, workflow and target.

True positive and negative values, false positive and negative values, sensitivity, and specificity for VIASURE SARS-CoV-2 Variant II (P681R+L452R) Real Time PCR Detection Kit for BD MAX™ System were calculated in relation to each comparator assay as shown in the following table:

Site	Comparator assay	Target	TP	TN	FP	FN	Sensitivity	Specificity
1	TaqPath COVID-19 CE-IVD RT-PCR Kit/ VIASURE SARS-CoV-2 Real Time PCR Detection Kit molecular assay + sequencing	P681R mutation	99	98	0	1	99% (93 – 99)	100% (95 – 100)
		L452R mutation	92	98	0	8	92% (84 – 96)	100% (95 – 100)

Table 9. True positive and negative values, false positive and negative values, sensitivity, specificity for VIASURE SARS-CoV-2 Variant II (P681R+L452R) Real Time PCR Detection Kit for BD MAX™ System.

In order to evaluate the compatibility of different sample matrices (nasopharyngeal swab, oropharyngeal swab and nasopharyngeal/oropharyngeal swab in Viral Transport Medium (VTM) from Vircell), a compatibility study have been carried out. The obtained results showed that the three different sample matrices were compatible with the VIASURE SARS-CoV-2 Variant II (P681R+L452R) Real Time PCR Detection Kit for BD MAX™ System.

The tentative clinical performance of VIASURE SARS-CoV-2 Variant II (P681R + L452R) Real Time PCR Detection Kit for BD MAX™ System with saliva samples was evaluated. Negative saliva single samples spiked with a known concentration of synthetic cDNA fragment for P681R mutation and L452R mutation in the S gene belonging to SARS-CoV-2 were tested. The evaluation was designed to be carried out with 20 positive samples (10 samples 2xLoD and 10 samples 10xLoD) and 10 negative samples. This assay was performed using a 750 µl sample volume of each condition added in the Sample Buffer Tube (SBT) of the TNA-3 Extraction Kit and it was run in full process mode (Automated extraction and PCR amplification) using BD MAX™ ExK™ TNA-3.

The percentage of agreement was calculated in relation to the expected result for each individual sample and results are showed in the following table.

Saliva sample	Agreement
Positive samples	95%
Negative samples	100%

Table 10. Percentage of agreement of VIASURE SARS-CoV-2 Variant II (P681R + L452R) Real Time PCR Detection Kit for BD MAX™ System with saliva samples.

Besides, a comparative analysis of nasopharyngeal swabs and saliva samples was carried out to evaluate the clinical performance of VIASURE SARS-CoV-2 Variant II (P681R + L452R) Real Time PCR Detection Kit for BD MAX™ System with saliva samples. 7 saliva samples and their corresponding nasopharyngeal sample were analysed and compared observing 100% of concordance. Both mutations (P681R and L452R) were detected in the six saliva samples characterized as Delta variant.

Target	TP	TN	FP	FN	Sensitivity	Specificity
P681R mutation	6	1	0	0	100% (51 – 100)	n.a*
L452R mutation	6	1	0	0	100% (51 – 100)	n.a*

Table 11. True positive and negative values, false positive and negative values, sensitivity, specificity for VIASURE SARS-CoV-2 Variant II (P681R+L452R) Real Time PCR Detection Kit for BD MAX™ System.

* Due to the limited availability of negative samples, the calculation of the clinical specificity of the test could not be performed.

In conclusion, saliva samples were compatible with VIASURE SARS-CoV-2 Variant II (P681R + L452R) Real Time PCR Detection Kit for BD MAX™ System.

Result show agreement to detect the P681R and L452R mutations using VIASURE SARS-CoV-2 Variant II (P681R+L452R) Real Time PCR Detection Kit for BD MAX™ System.

12.2. Analytical sensitivity

VIASURE SARS-CoV-2 Variant II (P681R+L452R) Real Time PCR Detection Kit for BD MAX™ System detection limit (LoD) results with a positive rate of $\geq 95\%$ are as follows:

- VIASURE SARS-CoV-2 Variant II (P681R+L452R) Real Time PCR Detection Kit for BD MAX™ System has a detection limit (LoD) of ≥ 40 RNA copies/reaction on nasopharyngeal samples and ≥ 250 RNA copies/reaction on saliva samples for P681R mutation.
- VIASURE SARS-CoV-2 Variant II (P681R+L452R) Real Time PCR Detection Kit for BD MAX™ System has a detection limit (LoD) of ≥ 40 RNA copies/reaction on nasopharyngeal samples and ≥ 500 RNA copies/reaction on saliva samples for L452R mutation.

Figure 2. Dilution series of SARS-CoV-2 Variant II (P681R mutation) (synthetic cDNA) (5.3×10^6 - 5×10^1 copies per reaction) template run on the BD MAX™ System (475/520 (FAM) channel).


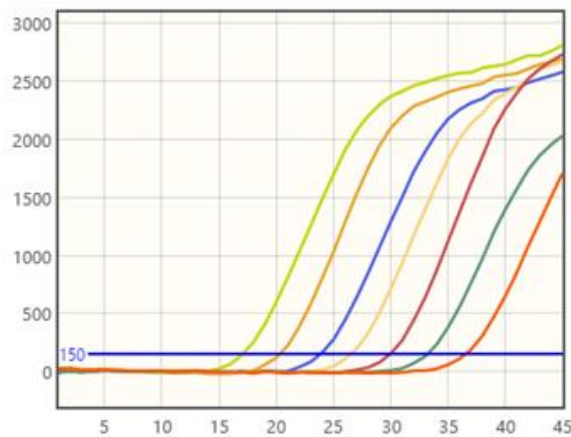


Figure 3. Dilution series of SARS-CoV-2 Variant II (L452R mutation) (synthetic cDNA) (5.3×10^6 - 5×10^1 copies per reaction) template run on the BD MAX™ System (530/565 (HEX) channel).

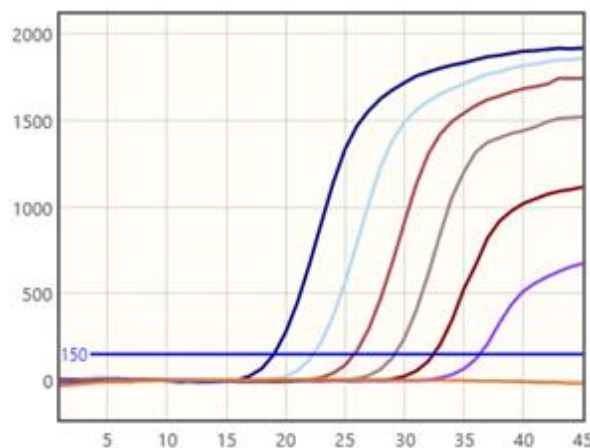

12.3. Analytical specificity

The specificity of the SARS-CoV-2 Variant II (P681R+L452R) assay was confirmed by testing a panel consisting of different microorganisms representing the most common respiratory pathogens. No cross-reactivity was detected between any of the following microorganisms tested:

Cross-reactivity testing					
Human Adenovirus types 1-5, 8, 15, 31, 40 and 41	-	Influenza A/Singapore/GP1908/2015, IVR-180 (H1N1)pdm09 virus	-	Human parainfluenza 1, 2, 3 and 4 viruses	-
Bocavirus	-	Influenza A/Thüringen/5/17 (H3N2) virus	-	Pneumocytis jirovecii Type A1 and g885652	-
Bordetella bronchiseptica	-	Influenza A/Switzerland/9715293/2013 (H3N2) virus	-	Human rhinovirus	-
Bordetella holmesii	-	Influenza A/Hong Kong/4801/2014, NYMC X-263B (H3N2) virus	-	Respiratory syncytial virus (RSV) A/B	-
Bordetella parapertussis	-	Influenza A/DE-SH/Reiherente/AR8444/ 2016 (H5N8) virus	-	Staphylococcus aureus	-
Bordetella pertussis	-	Influenza A/Anhui/1/2013 (H7N9) virus	-	Streptococcus pneumoniae	-
Chlamydia caviae	-	Influenza B/Brisbane/60/2008 virus	-	Streptococcus pyogenes	-
Chlamydia psittaci genotype A and C	-	Influenza A/South Australia/55/2014, IVR-175	-	SARS Coronavirus Strain Frankfurt 1	-
Chlamydophila pneumoniae CM-1	-	Influenza B/Phuket/3073/2013 virus	-	Human 2019-nCoV strain BetaCoV/Gemany/BavPat1/2020 p.1*	-
Human coronavirus 229E, OC43, NL63 and HKU1	-	Influenza B/Florida/04/06 virus	-	Human 2019-nCoV strain 2019-nCoV/Italy-INMI1*	-
MERS Coronavirus	-	Legionella bozemanii	-	MT007544.1 (SARS-CoV-2 isolate Australia/VIC01/2020)*	-
Enterovirus Coxsackievirus A24, A9 and B3	-	Legionella dumoffii	-	MN908947.3 (SARS-CoV-2 isolate Wuhan-Hu-1)*	-
Enterovirus Echovirus 30	-	Legionella longbeachae	-	SARS-CoV-2 strain 2019nCoV/USAWA1/2020*	-
Enterovirus 68, 71	-	Legionella micdadei	-	SARS-CoV-2 BetaCoV/Berlin/ChVir1670/2020_IsolatBER*	-
Haemophilus influenzae MinnA	-	Legionella pneumophila	-	SARS-CoV-2 BetaCoV/Munich/ChVir984/2020*	-
Influenza A/New Caledonia/20/99(H1N1) virus	-	Human metapneumovirus A and B	-	SARS-CoV-2 BetaCoV/Baden-Wuerttemberg/1/ChVir1577/2020_IsolatBER*	-
Influenza A/Victoria/210/2009 (H3N2)	-	Moraxella catarrhalis	-	SARS-CoV-2 B.1.1.7_710528 and SARS-CoV-2 B.1.1.7_601443 lineages (Alpha Variant) *	-
Influenza A/California/7/2009(H1N1) pdm09 virus	-	Mycoplasma pneumoniae	-	SARS-CoV-2 B.1.351 lineage (Beta Variant) *	-
Influenza A/Michigan/45/2015 (H1N1)pdm09 virus	-	Mycobacterium tuberculosis	-	SARS-CoV-2 P.1 lineage (Gamma Variant) *	-

Table 12. Reference pathogenic microorganisms used in this study.

* Please note that the detection of these SARS-CoV-2 strains is not considered in this assay. This test is designed for the qualitative detection of P681R mutation and L452R mutation in the S gene present in several SARS-CoV-2 variants.

12.4. Analytical reactivity

The reactivity of VIASURE SARS-CoV-2 Variant II (P681R+L452R) Real Time PCR Detection Kit for BD MAX™ System was evaluated against synthetic RNA controls from Kappa variant (B.1.617.1 India/CT-ILSGS00361/2021) and clinical samples characterized as Delta variant (B.1.617.2) by sequencing, showing positive results.

DANSK

1. Anvendelsesformål

VIASURE SARS-CoV-2 Variant II (P681R+L452R) Real Time PCR Detection Kit for BD MAX™ System er en automatiseret RT-PCR-test i realtid designet til kvalitativ påvisning af P681R-mutationen og L452R-mutationen i S-gen RNA fra SARS-CoV-2-positive nasofaryngeale/orofaryngeale og spytpøver.

Analysen er beregnet til at blive brugt med SARS-CoV-2 positive prøver eller, når testen udføres i forbindelse med VIASURE SARS-CoV-2 (N1 + N2) Real Time PCR Detection Kit for BD MAX™ System (Ref: 444215) med prøver fra patienter, der har mistanke om Coronavirus-sygdom 2019 (COVID-19) af deres sundhedspersonale (HCP).

Denne test er beregnet til at blive brugt som et hjælpemiddel til at overvåge forekomsten af varianter, der bærer P681R- eller L452R-mutationer i S-genet og til at hjælpe med kontrolforanstaltninger. Analysen anvender BD MAX™ System til automatisk ekstraktion af RNA og efterfølgende reeltids-RT-PCR med anvendelse af de medfølgende reagenser kombineret med universelle reagenser og engangsartikler til BD MAX™ System. RNA ekstraheres fra respirationsprøver og komplementær DNA (cDNA) syntetiseres og forstærkes ved hjælp af RT-PCR og detekteres ved hjælp af fluorescerende rapportørfarveprober, der er specifikke for P681R- og L452R-mutationer.

2. Oversigt og forklaring

Alle vira, herunder SARS-CoV-2, muterer over tid. nogle ændringer kan påvirke virussets egenskaber, såsom hvor let det spreder sig, den tilknyttede sygdoms sværhedsgrad eller ydeevnen af vacciner, terapeutiske lægemidler, diagnostiske værktøjer eller andre folkesundhedsmæssige og sociale foranstaltninger.

Udseendet af genmutationer er en naturlig og forventet begivenhed inden for udviklingsprocessen af en virus. Faktisk definerer nogle specifikke mutationer de virale genetiske grupper, som i øjeblikket cirkulerer globalt. Derudover var det, takket være den genetiske sekventering af patogenet rundt om i verden, muligt at etablere dispersionsmønstre og virusudvikling.

Ved udgangen af 2020 førte forekomsten af varianter forbundet med en højere risiko for folkesundheden til en karakterisering af interessante varianter (VOI) og problemvarianter (VOC) med henblik på at lette den epidemiologiske kontrol. Nogle af disse SARS-CoV-2-varianter er:

Varianterne Delta (B.1.617.2-stammen)- og Kappa (B.1.617.1-stamme) var tæt forbundet med en enorm stigning i COVID-19 i Indien i løbet af foråret 2021. Denne variant har flere mutationer i spikeproteinet, herunder P681R og L452R. Kappa-varianten har også genetiske mutationer i spike-proteinet, herunder P681R, L452R og E484Q.

Alle disse mutationer, der er beskrevet ovenfor, viser en potentiel reduktion i neutralisering ved visse immunterapier og en reduktion af vacciners forventede virkninger eller de er blevet identificeret til at forårsage smitteoverførsel i samfundet.

Udseendet på varianter, der øger overførbareheden af vira, dens virulens eller som undgår virkningen af neutraliserende antistoffer genereret efter den naturlige infektion eller vaccinen, udgør et første ordens folkesundhedsproblem, der kan have en vigtig indvirkning på kontrollen med pandemien.

Derfor er VIASURE SARS-CoV-2 Variant II (P681R+L452R) Real Time PCR Detection Kit for BD MAX™ System designet til at muliggøre detektion af hovedmutationen, der er forbundet med den variant, der overvåges.

3. Procedurens princip

VIASURE SARS-CoV-2 Variant II (P681R+L452R) Real Time PCR Detection Kit for BD MAX™ System er designet til kvalitativ påvisning af RNA med P681R og L452R-mutation i SARS-CoV-2 S-genet fra nasofaryngeale/orofaryngeale podedindsprøver og spytprøver. Detektionen foretages i et-trins realtids-RT-PCR-format, hvor den omvendte transskription og den efterfølgende forstærkning af den specifikke målsekvens finder sted i samme reaktionsrør. Det isolerede RNA-mål transskriberes, hvilket genererer komplementært DNA ved revers transkriptase, som efterfølges af amplifikation af et bevaret område af S-genet for SARS-CoV-2 for P681R-mutation og L452R-mutation ved hjælp af specifikke primere og fluorescerende-mærkede sonder.

VIASURE SARS-CoV-2 Variant II (P681R+L452R) Real Time PCR Detection Kit for BD MAX™ System baseret på 5' exonukleaseaktivitet fra DNA-polymerase. Under DNA-forstærkningen spaltes dette enzymproben, som er bundet til den komplementære DNA-sekvens og adskiller quencher-farvestoffet fra rapportøren. Denne reaktion genererer en stigning i det fluorescerende signal, som er proportional med mængden på måskabelonen. Denne fluorescens måles af BD MAX™ System.

VIASURE SARS-CoV-2 Variant II (P681R+L452R) Real Time PCR Detection Kit for BD MAX™ System indeholder i hvert rør alle de komponenter, der er nødvendige til realtids-PCR-analyse (specifikke primere/sonder, dNTPS, buffer, polymerase, omvendt transkriptase) i et stabiliseret format samt en endogen intern kontrol til overvågning af ekstraktionsprocessen og/eller hæmning af polymeraseaktiviteten. Analysen bruger et humant husholdningsgen som en endogen intern kontrol (IC) (humant RNase P-gen). Humane husholdningsgener er involveret i grundlæggende cellededdelighed og forventes derfor at være til stede i alle nukleerede humane celler og opretholde relativt konstante ekspressionsniveauer.

Mål	Kanal	Gen
P681R-mutation	475/520	S-gen
L452R-mutation	530/565	S-gen
Endogen intern kontrol (IC)	585/630	Menneskeligt RNase P-gen

Tabel 1. Mål, kanal og gener.

4. Leverede reagenser

VIASURE SARS-CoV-2 Variant II (P681R+L452R) Real Time PCR Detection Kit for BD MAX™ System indeholder følgende materialer og reagenser, som er beskrevet i Tabel 2:

Reagens/Materiale	Beskrivelse	Farve/stregkode	Mængde
SARS-CoV-2 Variant II (P681R+ L452R) reaction tube	En blanding af enzymer, primere sonder, buffere, dNTP'er, stabilisatorer og endogene interne kontroller i stabiliseret format	Blå folie	2 poser med 12 transparente rør
Rehydration Buffer tube	Opløsning til rekonstitution af det stabiliserede produkt	11 folie	1 pose med 24 transparente rør

Tabel 2. Reagenser og materialer leveret i VIASURE SARS-CoV-2 Variant II (P681R+L452R) Real Time PCR Detection Kit for BD MAX™ System med Kat. nr. VS-VAD124 (444218).

5. Reagenser og udstyr, der skal leveres af brugeren

Følgende liste omfatter materialer og udstyr, der er nødvendige til brug, men ikke inkluderet VIASURE SARS-CoV-2 Variant II (P681R+L452R) Real Time PCR Detection Kit for BD MAX™ System.

- Realtids-PCR-instrument: BD MAX™ System (Ref: 441916).
- BD MAX™ ExK™ TNA-3 (Ref:442827 or 442828).
- BD MAX™ PCR Cartridges (Ref: 437519).
- vortex.
- Mikropipetter (nøjagtighed mellem 2 og 1000 µl).
- Filterspidser.
- Pulverfrie engangshandsker
- (valgfrit: VIASURE SARS-CoV-2 (N1 + N2) Real Time PCR Detection Kit for BD MAX™ System (Ref: 444215)

6. Transport- og opbevaringsforhold

- Sættene kan sendes og opbevares ved 2 - 40 °C, indtil den udløbsdato, der er angivet på etiketten.
- Efter åbning af aluminiumsposerne, der indeholder reaktionsrørene, kan produktet bruges op til 28 dage.

7. Særlige forholdsregler for brugere

- Produktet er kun beregnet til brug af professionelle brugere, f.eks. laboratorie- eller sundhedspersonale og teknikere, der er uddannet i molekylærbiologiske teknikker.
- Til *in vitro*-diagnostisk brug.
- Brug ikke reagenser og/eller materialer, hvis udløbsdatoen er overskredet.
- Brug ikke sættet, hvis etiketten, der forsejler den ydre æske, er i stykker.
- Brug ikke reagenser, hvis beskyttelsesæskens er åben eller i stykker ved ankomsten.
- Brug ikke reagenser, hvis beskyttelsesposerne er åbne eller i stykker ved modtagelsen.
- Brug ikke reagenser, hvis tørremidlet ikke er til stede eller er i stykker inden i reagensposerne.
- Tørremidlet må ikke fjernes fra reagensposerne.
- Luk straks de beskyttende poser med reagenser med lynlåsforseglingen efter hver brug. Fjern eventuel overskydende luft i poserne inden forsejling.
- Brug ikke reagenser, hvis folien er blevet ødelagt eller beskadiget.
- Reagenser fra forskellige poser og/eller sæt og/eller partier må ikke blandes.
- Beskyt reagenser mod fugt. Længerevarende eksponering for fugt kan påvirke produktets ydeevne.
- Hold komponenterne væk fra lys.
- I tilfælde, hvor andre PCR-test udføres i det samme generelle område af laboratoriet, skal det sikres, VIASURE SARS-CoV-2 Variant II (P681R+L452R) Real Time PCR Detection Kit for BD MAX™ System, BD MAX™ ExK™ TNA-3 extraction kit, eventuelle yderligere reagenser, der er nødvendige til testen, og BD MAX™ System ikke er kontamineret. Undgå altid mikrobiel og ribonuklease (RNase) / deoxyribonuklease (DNase) kontaminering af reagenser. Det anbefales at anvende sterile RNase/DNase-fri aerosolresistente engangspipettespidser eller

positive fortrængningspipettespidser. Brug en ny spids til hver prøve. Handsker skal udskiftes før håndtering af reagenser og kassetter (BD MAX™ PCR Cartridge).

- For at undgå kontaminering af miljøet med amplikoner må BD MAX™ PCR Cartridge ikke brydes fra hinanden efter brug. Forseglingerne på BD MAX™ PCR Cartridge er designet til at forhindre kontaminering.
- Tilrettelæg en ensrettet arbejdsgang. Den skal begynde i ekstraktionsområdet og derefter flyttes til forstærknings- og detektionsområdet. Prøver, udstyr og reagenser må ikke returneres til det område, hvor det foregående trin blev udført.
- Følg god laboratoriepraksis. Brug beskyttelsestøj, engangshandsker, beskyttelsesbriller og maske. Man må ikke spise, drikke, ryge eller lægge makeup i arbejdsområdet. Vask hænder efter endt test.
- Prøverne skal behandles som potentielt smitsomme og/eller biologisk farlige, samt alle reagenser og materialer, der er blevet eksponeret for prøverne, og skal håndteres i overensstemmelse med de nationale sikkerhedsforskrifter. Træf de nødvendige forholdsregler under indsamling, opbevaring, behandling og bortskaffelse af prøver.
- Prøver og reagenser skal håndteres i et biologisk sikkerhedsskab. Anvend personlige værnemidler (PPE) i overensstemmelse med gældende retningslinjer for håndtering af potentielt smitsomme prøver. Affald bortskaffes i overensstemmelse med lokale retningslinjer.
- Regelmæssig dekontaminering af almindeligt anvendt udstyr anbefales, især mikropipetter og arbejdsflader.
- I overensstemmelse med Forordning (EF) nr. 1907/2006 (REACH), kræver VIASURE Real Time PCR Detection Kits ikke materialesikkerhedsdatablade (Material Safety Data Sheets) som en del af deres klassificering som værende ufarlige for helbredet og miljøet, fordi de ikke indeholder stoffer og/eller blandinger, som opfylder kriterierne for fareklassificering iht. forordning (EF) nr. 1272/2008 (CLP), eller forefindes i koncentrationer, der er højere end den værdi, der er angivet i den nævnte forordning til deres erklæring.
- Hvis sættet bruges i kombination med VIASURE SARS-CoV-2 (N1 + N2) Real-Time PCR Detection Kit for BD MAX System (Ref: 444215), se den tilhørende brugsanvisning.
- Se brugervejledningen til BD MAX™ System for yderligere advarsler, forholdsregler og procedurer.

8. Analysemetode

8.1. Prøveindsamling, opbevaring og transport

VIASURE SARS-CoV-2 Variant II (P681R+L452R) Real Time PCR Detection Kit for BD MAX™ System er blevet testet på nasopharyngeal pondepinde og spytp prøver, begge opsamlet i viralt transportmedium (VTM) - Vircell S.L. -; BD™ Universal Viral Transport (UVT) System media - BD - eller IMPROVIRAL™ Viral Preservative Medium (VPM) -Guangzhou Improve Medical Instruments Co. Ltd og oropharyngeal podninger opsamlet i viralt transportmedium (VTM) - Vircell. Andre typer prøver skal valideres af brugeren.

Prøveudtagning, opbevaring og transport skal vedligeholdes i overensstemmelse med de betingelser, der er valideret af brugeren. Samlet set skal åndedræts- og spytp prøver indsamles og mærkes på passende vis i rene beholdere med eller uden transportmidler (afhængigt af prøvetype) og behandles så hurtigt som muligt for at garantere testens kvalitet. Prøverne skal transporteres ved 2 til 8 °C i op til 72 timer i henhold til lokale og nationale bestemmelser for transport af patogen materiale. Ved langtidstransport (mere end 72 timer) anbefaler vi forsendelse ved ≤-20 °C eller lavere. Det anbefales at anvende friske prøver til testen. Prøverne kan opbevares ved

2 til 8 °C i op til 72 timer eller nedfryses ved -20 °C eller ideelt ved -70 °C for konservering. Gentagne fryse-tø-cykluser bør undgås for at forhindre nedbrydning af prøven og nukleinsyrer.

De nasofaryngeale/orofaryngeale podepindsprøver og spytpøverne skal indsamles, transporteres og opbevares i overensstemmelse med de relevante laboratorieretningslinjer. For yderligere oplysninger henvises til CDC guideline (CDC-retningslinjer for prøveudtagning. Websted <https://www.cdc.gov/urdo/downloads/SpecCollectionGuidelines.pdf> and Interim Guidelines for Collecting, Handling, and Testing Clinical Specimens for COVID-19. Websted <https://www.cdc.gov/coronavirus/2019-ncov/lab/guidelines-clinical-specimens.html>) og IDSA-retningslinje (Miller, J. M., Binnicker, M. J., Campbell, S.,... & Pritt, B. S. (2018). En vejledning i anvendelse af mikrobiologilaboratoriet til diagnosticering af smitsomme sygdomme: 2018 update by the Infectious Diseases Society of America and the American Society for Microbiology. *Kliniske infektionssygdomme*, 67(6), e1-e94).

8.2. Prøveklargøring og RNA-ekstraktion

Udfør prøveforberedelsen i overensstemmelse med anbefalingerne i brugsanvisningen til det anvendte ekstraktionssæt, BD MAX™ ExK™ TNA-3. Bemærk, at nogle andre prøver kan kræve forbehandling. Brugeren skal udvikle og validere ekstraktions- og præparationsprocedurer, der er specifikke til formålet.

Når du bruger prøver fra nasopharyngeal eller oropharyngeal podning:

1. Pipette mellem 400 og 750 µl nasofaryngeale/orofaryngeale podepinde opsamlet i virale transportmedier (VTM), i BD™ Universal Viral Transport (UVT) systemmedier eller IMPROVIRAL™ Viral Preservative Medium (VPM) ind i et BD MAX™ ExK™ TNA-3 Sample Buffer Tube, og luk røret med en septumhætte. Der sikres fuldstændig blanding ved at vortexe prøven ved høj hastighed i 1 minut. Fortsæt til BD MAX™ System Operation betjening.

I tilfælde af spytpøver, der skal indsamles i transportmedier:

1. Spytpøver kan opsamles i Viral Transport Medium (VTM), BD™ Universal Viral Transport (UVT) eller IMPROVIRAL™ Viral Preservative Medium (VPM) i et forhold på 1:3 (spyt:medie). Vortex i 1 minut ved høj hastighed. Der pipetteres 750 µl over i et BD MAX™ ExK™ TNA-3 Sample Buffer Tube, og røret lukkes med en septumhætte. Der sikres fuldstændig blanding ved at vortexe prøven ved høj hastighed i 1 minut. Fortsæt til BD MAX™ System Operation betjening.

Hvis der anvendes rene spytpøver:

1. Kombiner spyt med viralt transportmedium (VTM), BD™ Universal Viral Transport (UVT) eller IMPROVIRAL™ Viral Preservative Medium (VPM), så det endelige forhold mellem spyt:medie er 1:3. Vortex i 1 minut ved høj hastighed. Derefter pipetteres 750 µl opløsning over i et BD MAX™ ExK™ TNA-3 Sample Buffer Tube og røret lukkes med en septumhætte. Der sikres fuldstændig blanding ved at vortexe prøven ved høj hastighed i 1 minut. Fortsæt til BD MAX™ System Operation betjening.

8.3. PCR-protokol

Bemærk: Der henvises til brugervejledningen til BD MAX™ System for at få detaljerede instruktioner.

8.3.1. Oprettelse af PCR-testprogram til VIASURE SARS-CoV-2 Variant II (P681R+L452R) Real Time PCR Detection Kit for BD MAX™ System

Bemærk: Hvis du allerede har oprettet testen for VIASURE SARS-CoV-2 Variant II (P681R+L452R) Real Time PCR Detection Kit for BD MAX™ System kan du springe trin 8.3.1 over og gå direkte til 8.3.2.

- 1) Vælg fanen "Test Editor" (Testredigering) på skærmen "Run" (Kør) på BD MAX™ System
- 2) Klik på knappen "Create" (Opret).
- 3) I fanen Grundlæggende oplysninger i vinduet "Test Name" (testnavn) skal du navngive din test: VIASURE SARS-CoV-2 Variant II (P681R+L452R).
- 4) I rullemenuen "Extraction Type" (Ekstraktionstype), vælg "ExK TNA-3".
- 5) Vælg "Type 5" i rullemenuen "Master Mix Format".
 - a. Bemærk: Produktet kan bruges i kombination med VIASURE SARS-CoV-2 (N1 + N2) Real Time PCR Detection Kit for BD MAX™ System (Ref: 444215), vælg derefter "Dual Master Mix Concentrated Lyophilized MM with Rehydration Buffer (Type 5)". (Dual Master Mix Koncentreret Lyofiliseret MM med Rehydratiseringsbuffer, Type 5)
- 6) I "Sample extraction parameters" (Parametre for prøveekstraktion) vælges "User defined" (Brugerdefineret), og prøvevolumen justeres til 950 µl.
- 7) I "Ct Calculation" (Ct-beregning) vælges "Call Ct at Threshold Crossing" (Beregn Ct når tærsklen krydses).
- 8) Hvis du kører softwareversion 5.00 eller nyere, skal du vælge følgende konfiguration i "Custom Barcodes" (Brugerdefinerede strekkoder):
 - a. "Snap-In 2 Barcode" (Snap-In 2 strekkode): efterlad tom (vedrørende SARS-CoV-2 Variant II (P681R+L452R) reaction tube (reaktionsrør), der kræves ingen strekkodekonfiguration).
 - b. "Snap-In 3 Barcode" (Snap-In 3 strekkode): 11 (vedrørende Rehydration Buffer tube).
 - c. "Snap-In 4 Barcode" (Snap-In 4 strekkode): 1G, hvis det bruges i kombination med SARS-CoV-2 (N1 + N2) reaction tube (reaktionsrør) og formatet "Dual Master mix Concentrated Lyophilized MM with rehydration Buffer (Type 5)" (Dual Master Mix Koncentreret Lyofiliseret MM med Rehydratiseringsbuffer, Type 5) (Afsnit 8.3.1).
- 9) Indtast følgende parametre på fanen "PCR settings" (PCR-indstillinger): "Channel Settings" (Kanalindstillinger), "Gains" (Stigninger) og "Threshold" (Tærskel) (Tabel 3).
 - a. Bemærk: Produktet kan bruges i kombination med VIASURE SARS-CoV-2 (N1 + N2) Real Time PCR Detection Kit for BD MAX™ System (Ref: 444215), "PCR Settings" og "Test Steps" skal udfyldes for Snap-In 4 (blå) position (se den tilsvarende brugsanvisning).

Channel (Kanal)	Alias (Alias)	Gain (Gevinst)	Threshold (Tærskel)	Ct Min (Ct Min)	Ct Max (Ct Max)
475/520 (FAM)	P681R	80	150	0	40
530/565 (HEX)	L452R	80	150	0	40
585/630 (ROX)	IC	80	150	0	35
630/665 (Cy5)	-	0	0	0	0
680/715 (Cy5.5)	-	0	0	0	0

Tabel 3. "PCR settings" (PCR-indstillinger).

Bemærk: Det anbefales at angive minimumsgrænseværdierne angivet ovenfor for hver kanal som udgangspunkt, men de endelige indstillinger bør bestemmes af slutbrugeren ved fortolkning af resultaterne for at sikre, at tærskler falder inden for eksponentiel fase af fluorescenskurverne og over ethvert baggrundsignal. Tærskelværdien for forskellige instrumenter kan variere på grund af forskellige signalintensiteter.

- 10) I fanen "PCR settings" (PCR-indstillinger) indtastes følgende parametre samt "Spectral Cross Talk" (Spektral krydstale) (tabel 4).

		False Receiving Channel (Falsk modtagekanal)					
		Channel (Kanal)	475/520	530/565	585/630	630/665	680/715
Excitation Channel (Excitationskanal)	475/520	-	3,0	0,0	0,0	0,0	0,0
	530/565	1,0	-	0,0	0,0	0,0	0,0
	585/630	0,0	0,0	-	0,0	0,0	0,0
	630/665	0,0	0,0	0,0	-	0,0	0,0
	680/715	0,0	0,0	0,0	0,0	-	0,0

Tabel 4. Parametre for "Spectral Cross Talk" (spektral krydstale).

- 11) Indtast PCR-protokollen (tabel 5) på fanen "Test Steps" (Testtrin).

Step Name (Trinnavn)	Profile Type (Profiltype)	Cycles (Cyklusser)	Time (s) (Tid(er))	Temperature (Temperatur)	Detect (Registrering)
Reverse transcription (Revers transskription)	Hold	1	900	45 °C	-
Initial denaturation (Indledende denaturering)	Hold	1	120	98 °C	-
Denaturation and Annealing/Extension (Data collection) (Denaturering og annotering/udvidelse (dataindsamling))	2-temperatur	45	10	95 °C	-
			61,1	63 °C	✓

Tabel 5. PCR-protokol.


- 12) Klik på knappen "Save Test" (Gem test).

8.3.2. Opsætning af BD MAX™-stativ

- 1) For hver prøve, der skal testes, fjernes en samlet reagensstrimmel fra BD MAX™ ExK™ TNA-3 kit. Bank forsigtigt hver strimmel mod en hård overflade for at sikre, at alle væsker ligger i bunden af rørene, og anbring dem i BD MAX™ Systems prøvestativer.

- 2) Fjern det nødvendige antal BD MAX™ ExK™ TNA Extraction Tubes (B4) (hvid folie) fra deres beskyttelsespose. Sæt udtræksrør(-rørene) (hvid folie) i de tilsvarende positioner i TNA-strimlen (fastgør position 1, hvid farvekodning på stativet. Se Figur 1). Fjern overskydende luft, og luk posen med lynlåsforseglingen.
- 3) Bestem og adskil det passende antal SARS-CoV-2 Variant II (P681R+L452R) reaction tube (reaktionsrør) (blå folie), og klik dem på plads i deres tilsvarende positioner i strimlen (Snap-position 2, grøn farvekodning på stativet. Se Figur 1).
 - a. Fjern overskydende luft, og luk aluminiumsposerne med lynlåsforseglingen.
 - b. Rehydreringen udføres korrekt ved at sørge for, at det frysetørrede produkt ligger i bunden af røret og ikke er i kontakt med rørets top eller folieforseglingen. Bank forsigtigt hvert rør mod en hård overflade for at sikre, at alt produktet er i bunden af røret.
 - i. Bemærk: Hvis du vælger formatet "Dual Master Mix Concentrated Lyophilized MM with Rehydration Buffer (Type 5)" (Dual Master Mix Koncentreret Lyofiliseret MM med Rehydratiseringsbuffer (type 5) (afsnit 8.3.1), skal du bestemme og adskille det passende antal yderligere SARS-CoV-2 reaction tube (1G folie i tilfælde af VIASURE SARS -CoV-2 (N1 + N2) test) og klik ind i deres tilsvarende positioner i strimlen (Snap position 4, blå farvekodning på stativet. Se Figur 1). Fjern overskydende luft, og luk aluminiumsposerne med lynlåsforseglingen.
- 4) Fjern det nødvendige antal Rehydration Buffer tubes (11 folie), og klik dem fast på deres tilsvarende pladser på strimlen (klik-position 3, ikke-farvet kodning på stativet. Se Figur 1). Fjern overskydende luft, og luk posen med lynlåsforseglingen.
 - a. For at sikre, at overførslen udføres korrekt, skal man sørge for, at væsken ligger i bunden af røret og ikke er i kontakt med rørets top eller folieforseglingen. Bank forsigtigt på hvert rør på en hård overflade for at sikre, at al bufferen er i bunden af røret.

Figur 1. BD MAX™ TNA Reagent Strip (TNA) fra BD MAX™ ExK™ TNA-3 kit.

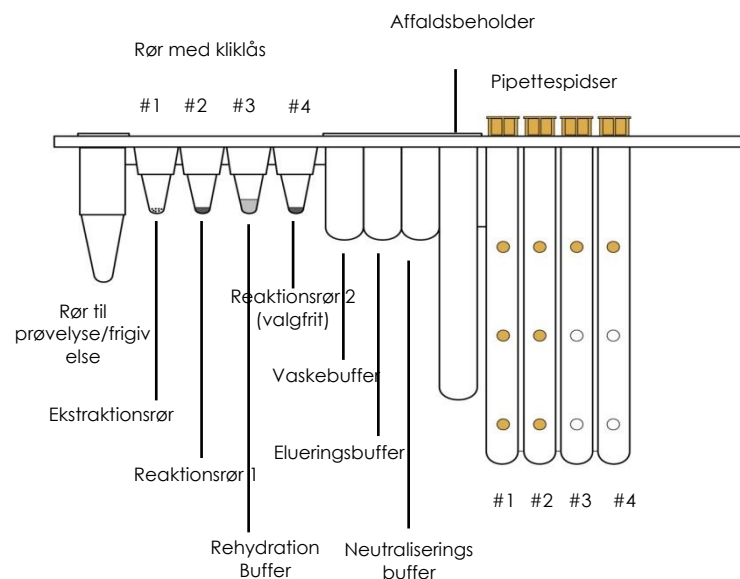

8.3.3. BD MAX™ Instrumentopsætning

- 1) Vælg fanen "Work List" (Arbejdsliste) på skærmen "Run" (Kør) på BD MAX™ Systemssoftware v4.50A eller nyere.
- 2) I rullemenuen "Test" skal du vælge *VIASURE SARS-CoV-2 Variant II (P681R+L452R)* (hvis den ikke allerede er oprettet, se afsnit 8.3.1).
- 3) Vælg det relevante lotnummer for kittet (fremgår af ekstraktionskittets udvendige æske) fra rullemenuen (valgfrit).
- 4) Indtast prøvebufferrørets identifikationsnummer i vinduet Sample tube (Prøverør) på Worklist (Arbejdsliste), enten ved at scanne strekkoden med scanneren eller ved manuel indtastning.
- 5) Udfyld prøven/patient-id'et og/eller adgangsvinduet på arbejdslisten, og klik på knappen "Save" (Gem). Fortsæt, indtil alle Sample Buffer Tubes (prøvebufferrør) er indtastet. Sørg for, at prøve-/patient-id'et og Sample Buffer Tubes matcher nøjagtigt.
- 6) Anbring det klargjorte Sample Buffer Tube i BD MAX™ Rack(s) (stativet/stativerne).
- 7) Sæt stativet/stativerne i BD MAX™ System (stativ A er placeret i venstre side af BD MAX™ System og stativ B i højre side).
- 8) Anbring det nødvendige antal BD MAX™ PCR Cartridges i BD MAX™ System.
- 9) Luk lågen til BD MAX™ System.
- 10) Klik på "Start Run" (Start procedure) for at starte proceduren.

8.3.4. BD MAX™ rapport

- 1) Klik på knappen "Results" (Resultater) i hovedmenuen.
- 2) Dobbeltklik enten på din kørsel på listen, eller tryk på knappen "View" (Vis).
- 3) Klik på "Print" (Udskriv), vælg: "Run Details, Test Details and Plot..." (Kør detaljer, testdetaljer og tegn grafik).
- 4) Klik på knappen "Print or Export" (Udskriv eller eksportér) på skærmbilledet Run Reports (Kør rapporter).

9. Tolkning af resultater

For en detaljeret beskrivelse af, hvordan man analyserer data, se BD MAX™ Systems brugervejledning.

Analyse af *VIASURE SARS-CoV-2 Variant II (P681R+L452R)* Real Time PCR Detection Kit for BD MAX™ System er beregnet til at blive udført som en refleks på prøver med positivt resultat for SARS-CoV-2 RNA. Hvis den bruges sammen med *VIASURE SARS-CoV-2 (N1 + N2)* Real Time PCR Detection Kit for BD MAX™ System på prøver af ukendt status for tilstedeværelse af SARS-CoV-2 RNA, henvises til brugsanvisningen for resultater fortolkning til bestemmelse af SARS-CoV-2 RNA-resultatet.

Analysen af data udføres som BD MAX™-software i overensstemmelse med producentens anvisninger. BD MAX™-softwaren rapporterer Ct-værdier og stigningskurver for hver detektor kanal for hver prøve, og testes på følgende måde:

- En Ct-værdi på 0 angiver, at der ikke blev beregnet nogen Ct-værdi af softwaren ved den angivne tærskelværdi (se tabel 3). En forstærkningskurve for prøven, der viser en Ct-værdi på "0", skal kontrolleres manuelt.

- Ct-værdien -1 angiver, at ingen forstærkningskurve er forekommet.

- Enhver anden Ct-værdi skal fortolkes i sammenhæng med forstærkningskurve og i overensstemmelse med retningslinjerne for tolkning af prøven som anført i Tabel 6.

Kontrollér, at det indvendige styresignal fungerer korrekt for amplifikationsblandingen. Desuden skal du kontrollere, at der ikke foreligger nogen rapport over BD MAX™ Systemfejl.

Resultaterne skal læses og analyseres ved hjælp af følgende tabel:

P681R-mutationsmål (475/520)	L452R-mutationsmål (530/565)	Endogenous Internal Control (585/630)	Fortolkning
+	-	+/- ¹	P681R-mutation fundet ¹
-	+	+/- ¹	L452R-mutation fundet ¹
+	+	+/- ¹	P681R-mutation og L452R-mutation fundet ¹
-	-	+ ¹	P681R-mutation og L452R-mutation ikke fundet ¹
-	-	- ²	Resultatet Unresolved (uløst) (UNR) optræder under tilstedeværelse af hæmmere i PCR-reaktionen eller når der opstår et overordnet problem (der ikke rapporteres med en fejlkode) under prøve kørslen og/eller forstærkningstrinnene.²
IND	IND	IND	Analyseresultatet er Indeterminate (ubestemmeligt) (IND). Skyldes en fejl i BD MAX™ System. Analyseresultat, der vises i tilfælde af en instrumentfejl, der knyttet til en fejlkode.
INC	INC	INC	Analyseresultatet er Incomplete (ufuldstændigt) (INC). Skyldes en fejl i BD MAX™ System. Analyseresultatet vises, hvor en fuldstændig kørsel ikke kunne gennemføres.

Tabel 6. Prøvefortolkning.

+: Der opstod forstærkning

-: Der opstod ingen forstærkning.

1 En prøve betragtes som positiv, hvis Ct-værdien er mindre end 40. Den endogene interne kontrol (IC) kan både vise et forstærkersignal eller intet forstærkersignal. Sommetider er IC-detektionen ikke nødvendig, fordi et højt kopinumner for målet kan forårsage præferenceamplifikation af mål-specifikke nukleinsyrer.

2 I tilfælde af P681R-mutation og L452R-mutation er målrettet mod steder, skal IC vise et forstærkningssignal med Ct mindre end 35. Ct-værdien kan være meget variabel på grund af den endogene interne kontrol er et humant rengøringsgen, der bør være til stede i alle humane kerneceller i den oprindelige prøve. Hvis der mangler signal eller Ct-værdi ≥ 35 for den endogene interne kontrol, betragtes resultatet som 'uløst', og det er nødvendigt at teste igen.

Resumé af mutationer forbundet med følgende slægter til stede i de mest kendte varianter af bekymring (VOC):

Stammer	WHO-mærke	Mutationer i S-genet ¹	
		P681R	L452R
B.1.617.1	Kappa	X	X
B.1.617.2	Delta	X	X

Tabel 7. Resumé af mutationer forbundet med kendte varianter af bekymring (VOC).

¹Sporing af SARS-CoV-2-varianter: <https://www.who.int/en/activities/tracking-SARS-CoV-2-variants/> (data op til 2. september 2021).

²Oversigt over SARS-CoV-2-varianter: <https://www.who.int/en/activities/tracking-SARS-CoV-2-variants/> (data op til 2. september 2021).

Andre varianter kan præsentere og mutationer P681R og L452R, fordi de ikke er specifikke for de nævnte varianter.

Den endelige tildeling til en afstamning skal udføres ved at sekventering.

I tilfælde af et fortsat tvetydigt resultat anbefales det at gennemgå brugsanvisningen, den ekstraktionsproces, som brugeren anvender; til at verificere den korrekte ydeevne for hvert RT-qPCR-trin og gennemgå parametrene og kontrollere kurvens sigmoide form og fluorescensintensiteten.

Resultaterne af testen bør vurderes af en læge på baggrund af anamnese, kliniske symptomer og andre diagnostiske tests.

10. Begrænsninger i testen

- Resultaterne af testen bør vurderes af en læge på baggrund af anamnese, kliniske symptomer og andre diagnostiske tests.
- Selv om denne test kan bruges sammen med andre typer prøver er den blevet valideret med nasofaryngeale/orofaryngeale pødepinde og spytpøver.
- For god testydeevne skal det frysetørrede produkt være i bunden af røret og ikke klæbe til det øverste område af røret eller folieforsøglingen. Bank forsigtigt hvert rør mod en hård overflade for at sikre, at alt produktet er i bunden af røret.
- Et udseende af reaktionsblandingen i stabiliseret format, som normalt findes i bunden af røret, forskelligt fra det sædvanlige (uden konisk form, inhomogent, mindre/større i størrelse og/eller farve forskellig fra hvidlig) ændrer ikke testens funktionalitet.
- Testens kvalitet afhænger af prøvens kvalitet; korrekt ekstraheret nukleinsyre fra luftvejsprøver skal ekstraheres.
- Denne test er en kvalitativ test og giver ikke kvantitative værdier eller angiver antallet af tilstedeværende organismer.
- Meget lave målniveauer under detektionsgrænsen kan påvises, men resultaterne er muligvis ikke reproducerbare.
- Prøver med en Ct-værdi på mellem 35 og 40 viser en større variabilitet i de resultater, der opnås.

- Der er mulighed for falske positive resultater på grund af krydskontaminering af SARS-CoV-2 RNA med P681R-mutationen eller L452R-mutationen i S-genet, eller prøver, der indeholder høje koncentrationer af mål-RNA eller kontaminering på grund af PCR-produkter fra tidligere reaktioner.
- De specifikke primer- og probekombinationer til påvisning af P681R-mutation eller L452R-mutation, der anvendes i VIASURE SARS-CoV-2 Variant II (P681R+L452R) Real Time PCR Detection Kit for BD MAX™ System, viser ikke signifikante kombinerede homologier med det humane genom, Menneskelig mikroflora eller andre coronavirus, som kan resultere i forudsigtelig falsk positiv.
- Falsk-negative resultater kan skyldes flere faktorer og kombinationer heraf, herunder:
 - Forkerte metoder til indsamling, transport, opbevaring og/eller håndtering af prøver.
 - Forkerte behandlingsprocedurer (herunder RNA-ekstraktion).
 - Nedbrydning af det virale RNA under forsendelse/opbevaring og/eller behandling af prøver.
 - Mutationer eller polymorfismer i primer- eller sondebindingsområder kan påvirke påvisningen af nye eller ukendte SARS-CoV-2-varianter.
 - En virusmængde i prøven under detektionsgrænsen for analysen.
 - Tilstedeværelsen af RT-qPCR-hæmmere eller andre typer interfererende stoffer. Virkningerne af vacciner, antivirale terapeutiske midler, antibiotika, kemoterapeutika eller immunsuppressive lægemidler, der anvendes til at forebygge COVID-19 eller under behandlingen af infektionen, er ikke blevet evalueret.
 - Manglende overholdelse af brugsanvisningen og analyseproceduren.
- Nogle prøver kan undlade at udvise RNase P-amplifikationskurver på grund af lave humane celletal i den oprindelige kliniske prøve. Et negativt IC-signal udelukker ikke tilstedeværelsen af P681R-mutationen eller L452R-mutationen i en klinisk prøve.
- Et positivt testresultat indikerer ikke nødvendigvis tilstedeværelsen af levedygtige vira og betyder ikke, at disse vira er smitsomme eller forårsager kliniske symptomer. Et positivt resultat indikerer imidlertid tilstedeværelsen af målvirussekvenser.
- Tilstedeværelsen af P681R- og L452R-mutationer er forbundet med Kappa (stamme B.1.617.1) og Delta (stamme B.1.617.2)-varianter, men endelig tildeling til en stamme skal ske ved sekventering.
- Negative resultater udelukker ikke tilstedeværelse af SARS-CoV-2 RNA på grund af denne analyse er beregnet til at blive brugt med positive SARS-CoV-2-prøver.
- Hvis der opnås uafklarede, ubestemte eller ufuldstændige resultater ved hjælp af VIASURE SARS-CoV-2 Variant II (P681R+L452R) Real-Time PCR Detection Kit for BD MAX™ System, kræves en ny test. Uløste resultater kan skyldes tilstedeværelsen af hæmmere i prøven eller forkert rehydrering af frysetørrede reaktionsblandingsrør. Hvis der opstår en instrumentfejl, kan det medføre ubestemmelige eller ufuldstændige resultater.

11. Kvalitetskontrol

VIASURE SARS-CoV-2 Variant II (P681R+L452R) Real Time PCR Detection Kit for BD MAX™ System indeholder en intern endogen kontrol (IC) i hvert reaktionsrør, der bekræfter korrekt teknikydelse.

12. Ydelseskarakteristika

12.1. Klinisk sensitivitet og specificitet

Den kliniske ydeevne af VIASURE SARS-CoV-2 Variant II (P681R+L452R) Real Time PCR Detection Kit for BD MAX™ System blev testet ved hjælp af kliniske prøver (nasopharyngeale podepinde), der allerede var karakteriseret som positive eller negative for SARS-CoV-2, fra patienter. Resultaterne var følgende:

	Center	Prøvetype	Arbejdsgang	Mål
1	CerTest Biotec S.L (Zaragoza, Spain)	nasopharyngeal podepind	BD MAX™ ExK™ TNA-3 kit + BD MAX™ System	P681R-mutation
				L452R-mutation

Tabel 8. Sted, prøvetype, arbejdsgang og mål.

Sand-positive og -negative værdier, falsk-positive og -negative værdier, følsomhed og specificitetsværdier for VIASURE SARS-CoV-2 Variant II (P681R+L452R) Real Time PCR Detection Kit for BD MAX™ System™ blev beregnet i forhold til hver komparatoranalyse som vist i følgende tabel:

Center	Komparatoranalyse	Mål	TP	TN	FP	FN	Følsomhed	Specificitet
1	Molekylær test TaqPath COVID-19 CE-IVD RT-PCR Kit / VIASURE SARS-CoV-2 Real Time PCR Detection Kit+ sekventering	P681R-mutation	99	98	0	1	99% (93 – 99)	100% (95 – 100)
		L452R-mutation	92	98	0	8	92% (84 – 96)	100% (95 – 100)

Tabel 9. Sand-positive (TP) eller -negative værdier(TN), falsk-positive (FP) og -negative værdier (FN), sensitivitet, specificitet, -- værdier VIASURE SARS-CoV-2 Variant II (P681R+L452R) Real Time PCR Detection Kit for BD MAX™ System.

For at vurdere kompatibiliteten mellem forskellige prøvematrixer (nasopharyngeal podning, oropharyngeal podning og nasopharyngeal/oropharyngeal podning i Viral Transport Medium (VTM) fra Vircell) blev der udført en kompatibilitetsundersøgelse. De opnåede resultater viste, at de tre forskellige prøvematrixer var kompatible med VIASURE SARS-CoV-2 Variant II (P681R+L452R) Real Time PCR Detection Kit for BD MAX™ System.

Ydeevnen for VIASURE SARS-CoV-2 Variant II (P681R + L452R) Real Time PCR Detection Kit for BD MAX™ System med spytp prøver blev evalueret. Negative enkeltprøver af spyt tilsat en kendt koncentration af syntetisk cDNA-fragment for P681R-mutationen og L452R-mutationen i S-genet tilhørende SARS-CoV-2 blev analyseret. Evalueringen blev designet til at blive udført med 20 positive prøver (10 prøver 2xLoD og 10 prøver 10xLoD) og 10 negative prøver. Denne analyse blev udført ved hjælp af et prøveeksemplarvolumen på 750 af hver tilstand, der blev tilføjet til Sample Buffer Tube (SBT) i TNA-3 Extraction Kit, og det blev kørt i fuld proces tilstand (automatiseret ekstraktion og PCR-forstærkning) under anvendelse af BD MAX™ ExK™ TNA-3.

Procentdelen af overensstemmelse blev beregnet i forhold til det forventede resultat for hver enkelt prøve, og resultaterne vises i den nedenstående tabel.

Spytprøve	Overensstemmelse
Positive prøver	95%
Negative prøver	100%

Tabel 10. Ydeevnen for VIASURE SARS-CoV-2 Variant II (P681R + L452R) Real Time PCR Detection Kit for BD MAX™ System med spytp prøver.

Desuden blev der udført en sammenlignende analyse af nasopharyngeale pødepinde og spytpøver for at evaluere den kliniske ydeevne af VIASURE SARS-CoV-2 Variant II (P681R + L452R) Real Time PCR Detection Kit for BD MAX™ System med spytpøver. 7 spytpøver og deres tilsvarende nasopharyngeale prøve blev analyseret og sammenlignet ved at observere 100 % af konkordansen. Begge mutationer (P681R og L452R) blev påvist i de seks spytpøver karakteriseret som Delta-variant.

Mål	TP	TN	FP	FN	Følsomhed	Specificitet
P681R-mutation	6	1	0	0	100% (51 – 100)	ikke relevant*
L452R-mutation	6	1	0	0	100% (51 – 100)	ikke relevant*

Tabel 11. Sand-positive (TP) eller -negative værdier (TN), falsk-positive (FP) og -negative værdier (FN), sensitivitet, specificitet, --værdier VIASURE SARS-CoV-2 Variant II (P681R+L452R) Real Time PCR Detection Kit for BD MAX™ System.

*Fordi negative prøver ikke blev analyseret, kunne beregningen af testens specificitet ikke udføres.

Det blev konkluderet, at spytpøver er kompatible med VIASURE SARS-CoV-2 Variant II (P681R + L452R) Real Time PCR Detection Kit for BD MAX™ System.


De opnåede resultater viste, at de tre forskellige prøvematrixer var kompatible med VIASURE SARS-CoV-2 Variant II (P681R+L452R) Real Time PCR Detection Kit for BD MAX™ System.

12.2. Analytisk sensitivitet


VIASURE SARS-CoV-2 Variant II (P681R+L452R) Real Time PCR Detection Kit for BD MAX™ System detekteringsgrænse (LoD) -resultater med en positiv sats på $\geq 95\%$ er som følger:

- VIASURE SARS-CoV-2 Variant II (P681R+L452R) Real Time PCR Detection Kit for BD MAX™ System har en detektionsgrænse (LoD) på ≥ 40 genom/reaktionskopier i nasopharynx-prøver og ≥ 250 genom/reaktionskopier i spytpøver til P681R-mutation.
- VIASURE SARS-CoV-2 Variant II (P681R+L452R) Real Time PCR Detection Kit for BD MAX™ System har en detektionsgrænse (LoD) på ≥ 40 genom/reaktionskopier i nasopharynx-prøver og ≥ 500 genom/reaktionskopier i spytpøver til L452R-mutation.

Figur 2. Fortyndingsserie af SARS-CoV-2 Variant II(P681R) cDNA ($5,3 \cdot 10^6$ - $5 \cdot 10^1$ genomkopier pr. reaktion) kører på BD MAX™ System (475/520 (FAM) -kanalen).

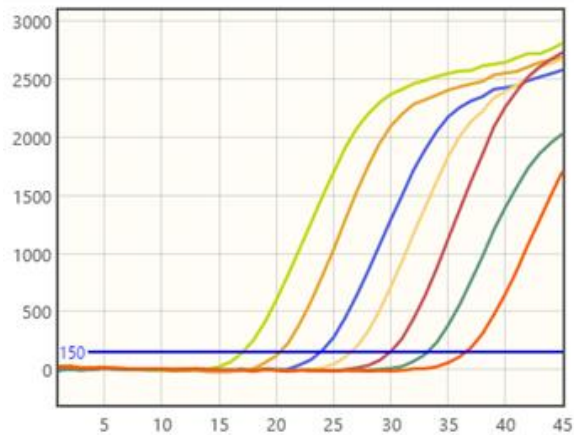

Figur 3. Fortyndingsserie af SARS-CoV-2 Variant II (L452R-mutation) II (syntetisk cDNA) ($5,3 \cdot 10^6$ - $5 \cdot 10^1$ genomkopier pr. reaktion) skabelon kørt på BD MAX™ System (530/565 (HEX) -kanalen).

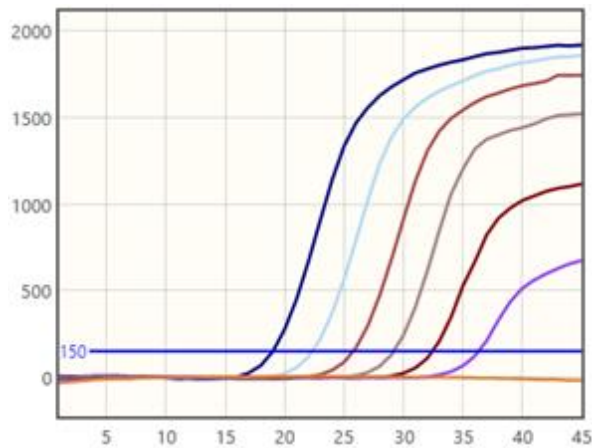

12.3. Analytisk specificitet

Specificiteten af SARS-CoV-2 Variant II (P681R+L452R)-analysen blev bekræftet ved at teste et panel bestående af forskellige mikroorganismer, der repræsenterer de mest almindelige respiratoriske patogener. Der blev ikke påvist krydsreaktivitet mellem nogen af følgende testede mikroorganismer:

Krydsreaktivitetstest					
Human Adenovirus-type 1-5, 8, 15, 31, 40 og 41	-	Influenza A/Singapore/GP1908/2015, IVR-180 (H1N1)pdm09-virus	-	Menneskelig parainfluenza 1, 2, 3 og 4 vira	-
Bocavirus	-	Influenza A/Thüringen/5/17 (H3N2)-virus	-	Pneumocytis jirovecii Type A1 og g885652	-
Bordetella bronchiseptica	-	Influenza A/Switzerland/9715293/2013 (H3N2)-virus	-	Menneskelig rhinovirus	-
Bordetella holmesii	-	Influenza A/Hong Kong/4801/2014, NYMC X-263B (H3N2)-virus	-	Respiratorisk syncytialvirus (RSV) A/B	-
Bordetella parapertussis	-	Influenza A/DE-SH/Reiherente/AR8444/ 2016 (H5N8)-virus	-	Staphylococcus aureus	-
Bordetella pertussis	-	Influenza A/Anhui/1/2013 (H7N9)-virus	-	Streptococcus pneumoniae	-
Chlamydia caviae	-	Influenza B/Brisbane/60/2008-virus	-	Streptococcus pyogenes	-
Chlamydia psittaci genotype A og C	-	Influenza A/South Australia/55/2014, IVR-175	-	SARS Coronavirus-stamme Frankfurt 1	-
Chlamydophila pneumoniae CM-1	-	Influenza B/Phuket/3073/2013 virus	-	Menneskelig stamme 2019-nCoV BetaCoV/Tyskland/BavPat1/2020 s.1*	-
Menneskelig coronavirus 29E OC43, NL63 og HKU1	-	Influenza B/Florida/04/06-virus	-	Menneskelig 2019-nCoV-stamme 2019-nCoV/Italy-INMI1*	-
MERS Coronavirus	-	Legionella bozemanii	-	MT007544.1 (SARS-CoV-2 isolat Australia/VIC01/2020)*	-
Enterovirus Cocksackievirus A24, A9 og B3	-	Legionella dumoffii	-	MN908947.3 (SARS-CoV-2 isolat Wuhan-Hu-1)*	-
Enterovirus Echovirus 30	-	Legionella longbeachae	-	SARS-CoV-2 stamme 2019nCoV/USAWA1/2020*	-
Enterovirus 68 , 71	-	Legionella micdadei	-	SARS-CoV-2 BetaCoV/Berlin/ChVir1670/2020_IsolatBER*	-
Haemophilus influenzae MinnA	-	Legionella pneumophila	-	SARS-CoV-2 BetaCoV/Munich/ChVir984/2020*	-
Influenza A/New Caledonia/20/99(H1N1)-virus	-	Menneskelig t metapneumovirus A og B	-	SARS-CoV-2 BetaCoV/Baden-Wuerttemberg/1/ChVir1577/2020_IsolatBER*	-
Influenza A/Victoria/210/2009 (H3N2)	-	Moraxella catarrhalis	-	SARS-CoV-2 B.1.1.7_710528 og SARS-CoV-2 B.1.1.7_601443 afstamninger (Alpha Variant) *	-
Influenza A/California/7/2009(H1N1) pdm09-virus	-	Mycoplasma pneumoniae	-	SARS-CoV-2 B.1.351 stamme (Beta Variant) *	-
Influenza A/Michigan/45/2015 (H1N1)pdm09-virus	-	Mycobacterium tuberculosis	-	SARS-CoV-2 p.1-stamme (Gamma-variant) *	-

Tabel 12. Referencepatogene mikroorganismer, der blev brugt i denne undersøgelse.

*Bemærk, at detektion af disse SARS-CoV-2-stammer ikke overvejes i denne analyse. Denne test er designet til kvalitativ påvisning af P681R-mutation og L452R-mutation i S-genet i flere SARS-CoV-2-varianter.

12.4. Analytisk reaktivitet











Reaktiviteten af VIASURE SARS-CoV-2 Variant II (P681R+L452R) Real Time PCR Detection Kit for BD MAX™ System blev evalueret mod syntetiske RNA-kontroller fra Kappa-variant (B.1.617.1 Indien/CT-ILSGS00361/2021) og kliniske prøver karakteriseret som Delta-variant (B.1.617.2) ved sekventering, der viste positive resultater.

Bibliography/ Bibliografi

1. Huang, C. *et al.* Clinical features of patients infected with 2019 novel coronavirus in Wuhan, China. *The Lancet*, 2020. DOI : 10.1016/S0140-6736(20)30183-5.
2. Zhu N. *et al.* A novel coronavirus from patients with pneumonia in China, 2019. *New England Journal of Medicine.*, 2020. DOI : 10.1056/NEJMod2001017.
3. World Health Organization. MERS situation update. January 2020. Available from <https://applications.emro.who.int/docs/EMCSR254E.pdf?ua=1> Accessed June 2021.
4. Chen N. *et al.*. Epidemiological and Clinical Characteristics of 99 Cases of 2019-Novel Coronavirus (2019-nCoV) Pneumonia in Wuhan, China. *The Lancet*, 2020. DOI: 10.1016/S0140-6736(20)30211-7.
5. Lv D.F. *et al.* Dynamic change process of target genes by RT-PCR testing of SARS-Cov-2 during the course of a Coronavirus Disease 2019 patient. *Clinica Chimica Acta* 2020; 506: 172-175.
6. World Health Organization. Clinical management of COVID-19 disease" Interim guidance 27 May 2020. Available from <https://www.who.int/publications/i/item/clinical-management-of-covid-19> Accessed June 2021.
7. Lu R. *et al.* Genomic characterisation and epidemiology of 2019 novel coronavirus: implications for virus origins and receptor binding. *The Lancet*, 2020. DOI : 10.1016/S0140-6736(20)30251-8.
8. Rothe C. *et al.* Transmission of 2019-nCoV Infection from an Asymptomatic Contact in Germany. *New England Journal of Medicine*, 2020. DOI : 10.1056/NEJMc2001468.
9. Centers of Disease Control and Prevention (CDC). Coronavirus Disease 2019 (COVID-19), Older Adults. Available from <https://www.cdc.gov/coronavirus/2019-ncov/need-extra-precautions/older-adults.html> Accessed August 2021.
10. World Health Organization. Laboratory testing for 2019 novel coronavirus (2019-nCoV) in suspected human cases. Interim guidance. 19 March 2020. Available from <https://www.who.int/publications-detail/laboratory-testing-for-2019-novel-coronavirus-in-suspected-human-cases-20200117> Accessed June 2021.
11. Yan Y *et al.* Laboratory testing of SARS-CoV, MERS-CoV, and SARS-CoV-2 (2019-nCoV): Current status, challenges, and countermeasures. *Reviews in Medical Virology* 2020; 30(3):e2106.
12. Centers of Disease Control and Prevention (CDC). 2019-Novel Coronavirus (2019-nCoV) Real-time rRT-PCR Panel Primers and Probes. <https://www.cdc.gov/coronavirus/2019-ncov/downloads/rt-pcr-panel-primer-probes.pdf> Accessed June 2021.
13. Chu D.K.W. *et al.* Molecular Diagnosis of a Novel Coronavirus (2019-nCoV) Causing an Outbreak of Pneumonia. *Clinical Chemistry* 2020;66(4): 549-555.
14. Corman V.M. *et al.* Detection of 2019 novel coronavirus (2019-nCoV) by real-time RT-PCR. *European communicable disease bulletin* 2020;25(3).
15. European Centre for Disease Prevention and Control. Novel coronavirus disease 2019 (COVID-19) pandemic: increased transmission in the EU/EEA and the UK – sixth update – 12 March 2020. Stockholm: ECDC; 2020. Available from <https://www.ecdc.europa.eu/sites/default/files/documents/RRA-sixth-update-Outbreak-of-novel-coronavirus-disease-2019-COVID-19.pdf> Accessed June 2021.
16. Lim, Y. X., Ng, Y. L., Tam, J. P., & Liu, D. X. (2016). Human coronaviruses: a review of virus–host interactions. *Diseases*, 4(3), 26.
17. McBride R. *et al.* The coronavirus nucleocapsid is a multifunctional protein. *Viruses* 2014; 6(8):2991-3018.
18. Sheikh A. *et al.* Analysis of preferred codon usage in the coronavirus N genes and their implications for genome evolution and vaccine design. *Journal of Virological Methods* 2020; 277:113806.

19. World Health Organization. Public health surveillance for COVID-19. 16 December 2020. Available from [https://www.who.int/publications-detail/global-surveillance-for-human-infection-with-novel-coronavirus-\(2019-ncov\)](https://www.who.int/publications-detail/global-surveillance-for-human-infection-with-novel-coronavirus-(2019-ncov)) Accessed June 2021.
20. Enfermedad por coronavirus, COVID-19, Información Científica-técnica. Centro de Coordinación de Alertas y Emergencias Sanitarias. Ministerio de Sanidad, España. 01-2021.
21. Centers of Disease Control and Prevention (CDC). Emerging SARS-CoV-2 Variants. Available from <https://www.cdc.gov/coronavirus/2019-ncov/science/science-briefs/scientific-brief-emerging-variants.html> Accessed June 2021.
22. Centers of Disease Control and Prevention (CDC). SARS-CoV-2 Variant Classifications and Definitions. Available from <https://www.cdc.gov/coronavirus/2019-ncov/cases-updates/variant-surveillance/variant-info.html> Accessed August 2021.

Symbols for IVD components and reagents/ Symboler for IVD-komponenter og -reagenser

 <i>In vitro</i> diagnostic device In vitro-diagnostisk udstyr	 Keep dry Opbevares tørt	 Use by Anvendes inden	 Manufacturer Producent	 Batch code (Lot) Batch-kode (parti)
 Consult instructions for use Se brugsanvisningen	 Temperature limitation Temperaturbegrænsning	 Contains sufficient for <n> test Indeholder nok til <n> tests	 Sample diluent Prøvefortynding	 Catalog number Katalognummer

Trademarks

BD MAX™ is a registered trademark of Becton, Dickinson and Company.

Change Control / Ændringskontrol		
Version No. / Versionsnr.	Changes / Ændringer	Date / Dato
00	Original version / Original version.	26/10/2021

Table A 2. Control change table/ Tabel over ændringskontrol.

Revision: 26 Ottobre 2021

VIASURE



CerTest Biotec, S.L.

Pol. Industrial Río Gállego II · Calle J, Nº1
50840, San Mateo de Gállego, Zaragoza (Spain)

Tel. (+34) 976 520 354

Fax (+34) 976 106 268

certest@certest.es | viasure@certest.es

www.certest.es

One step ahead



F-566 rev01

